

Fig. 1

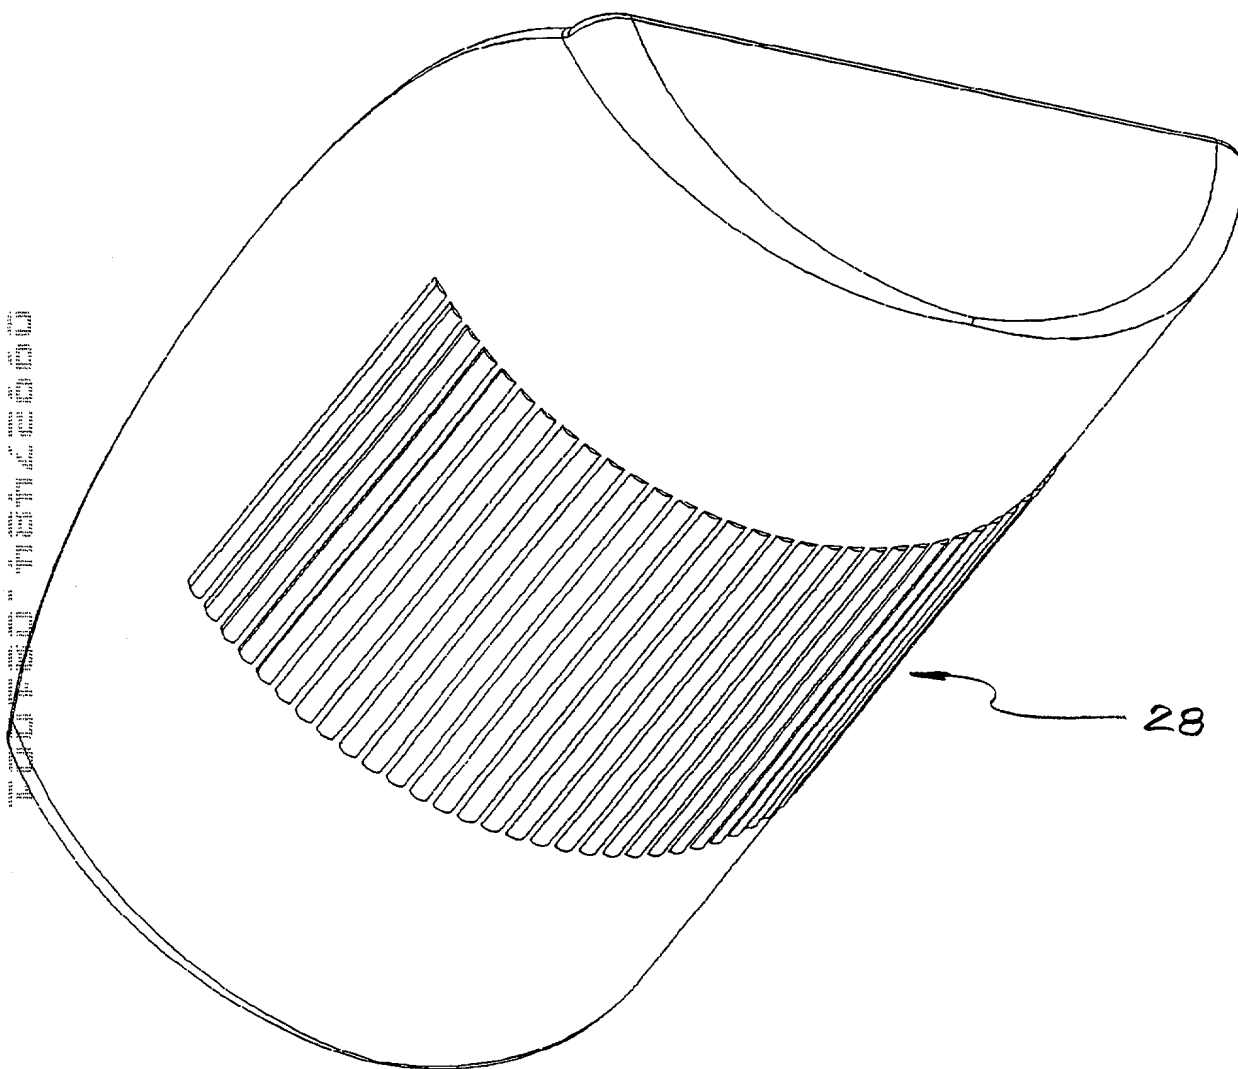


Fig. 2

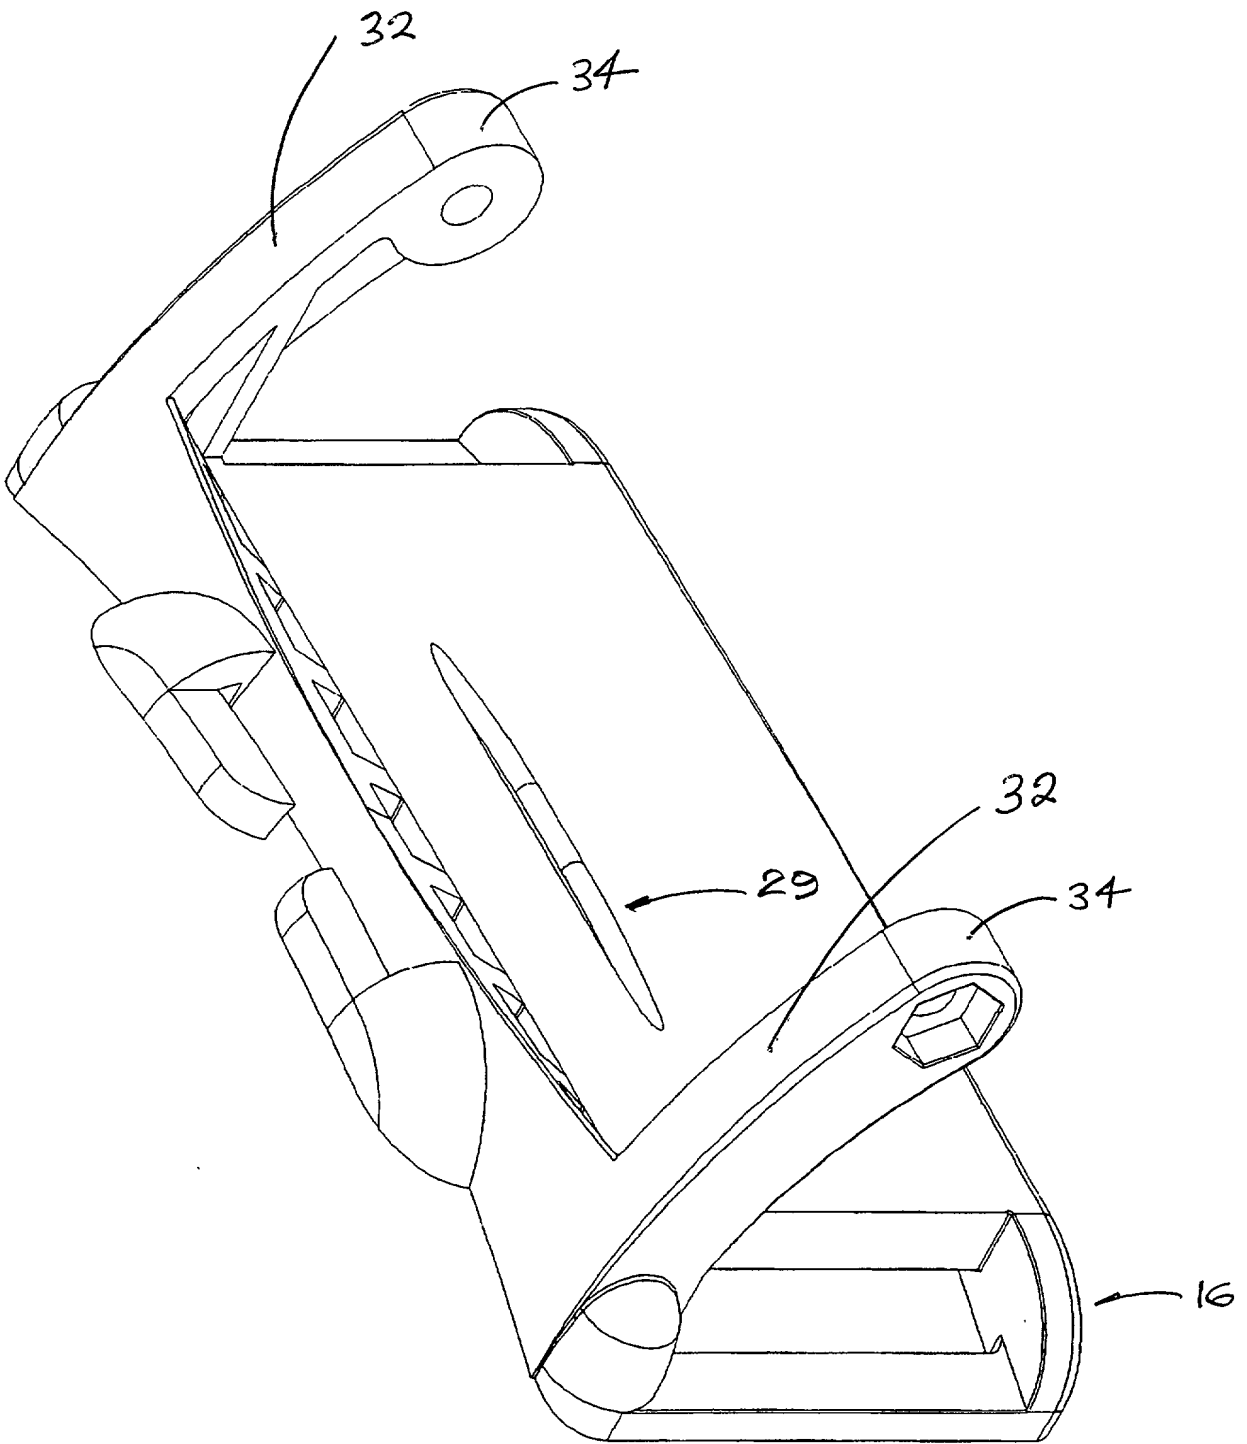


Fig. 3

FIG. 4 is a perspective view of the device 100 in an open position, showing the housing 110, the lid 120, the handle 130, the trigger 140, the button 150, the spring 160, the plunger 170, the needle 180, the needle guard 190, the needle holder 200, the needle cap 210, the needle cap holder 220, and the needle cap cap 230.

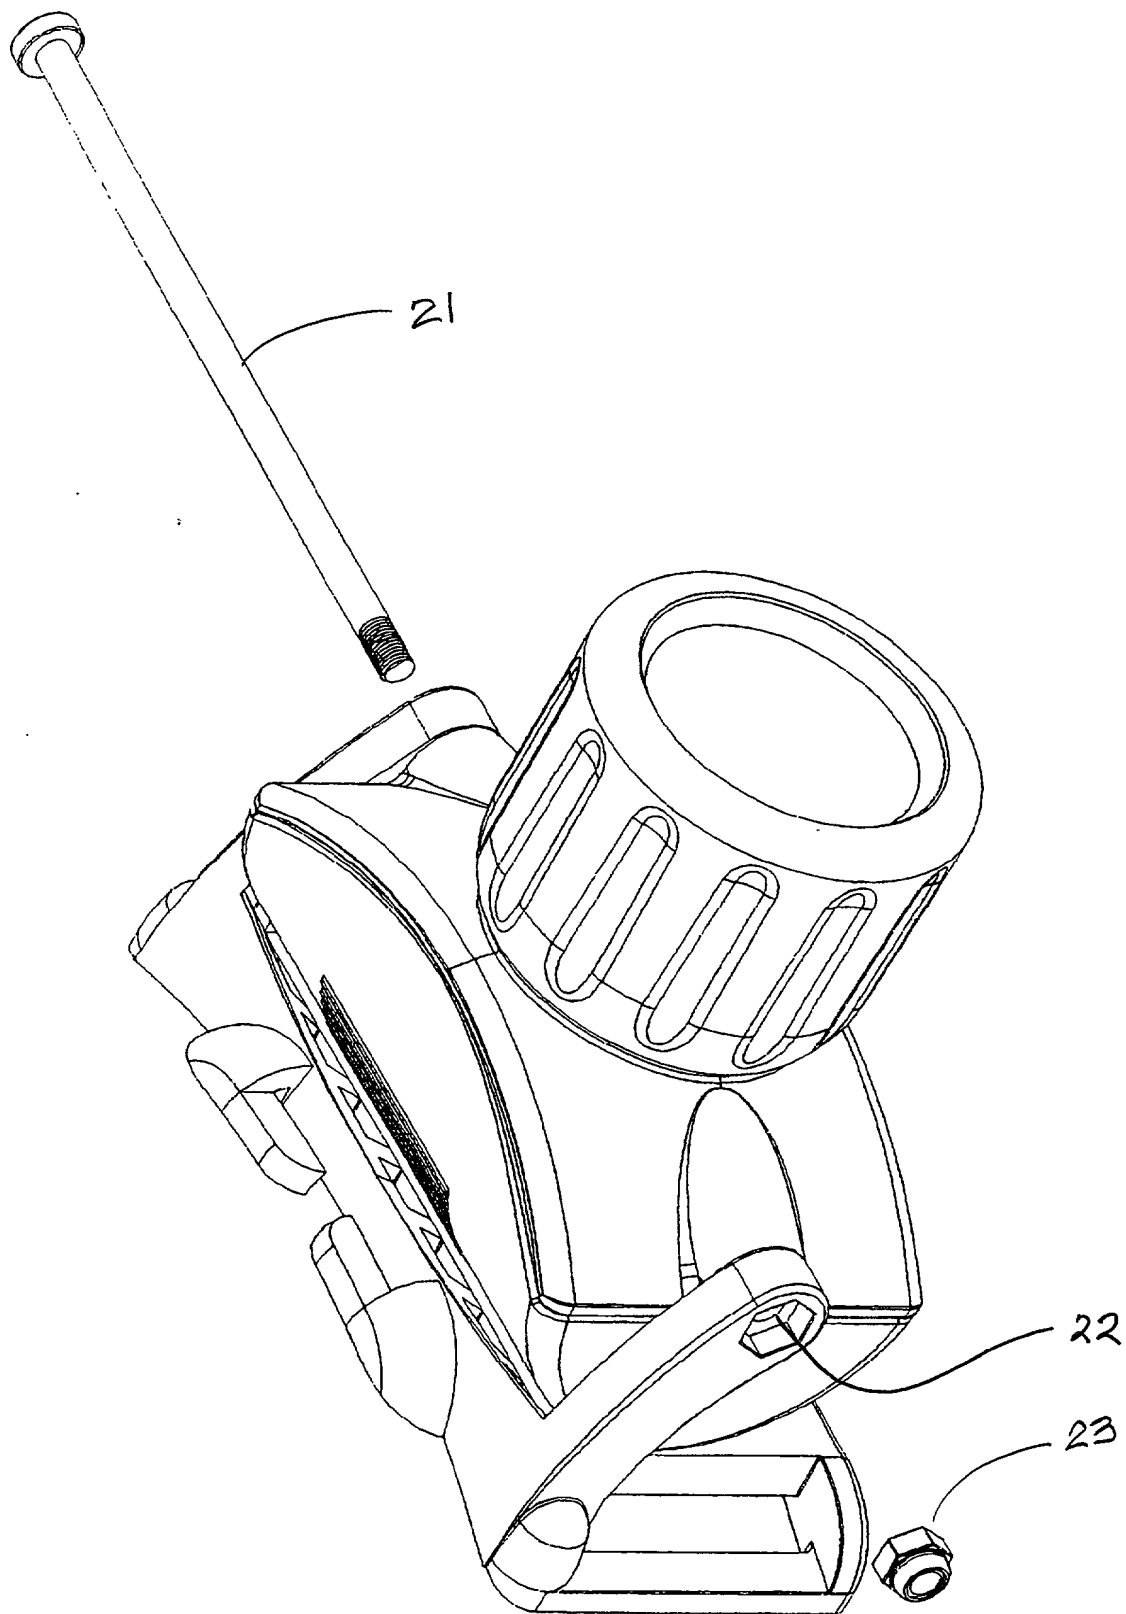


Fig. 4

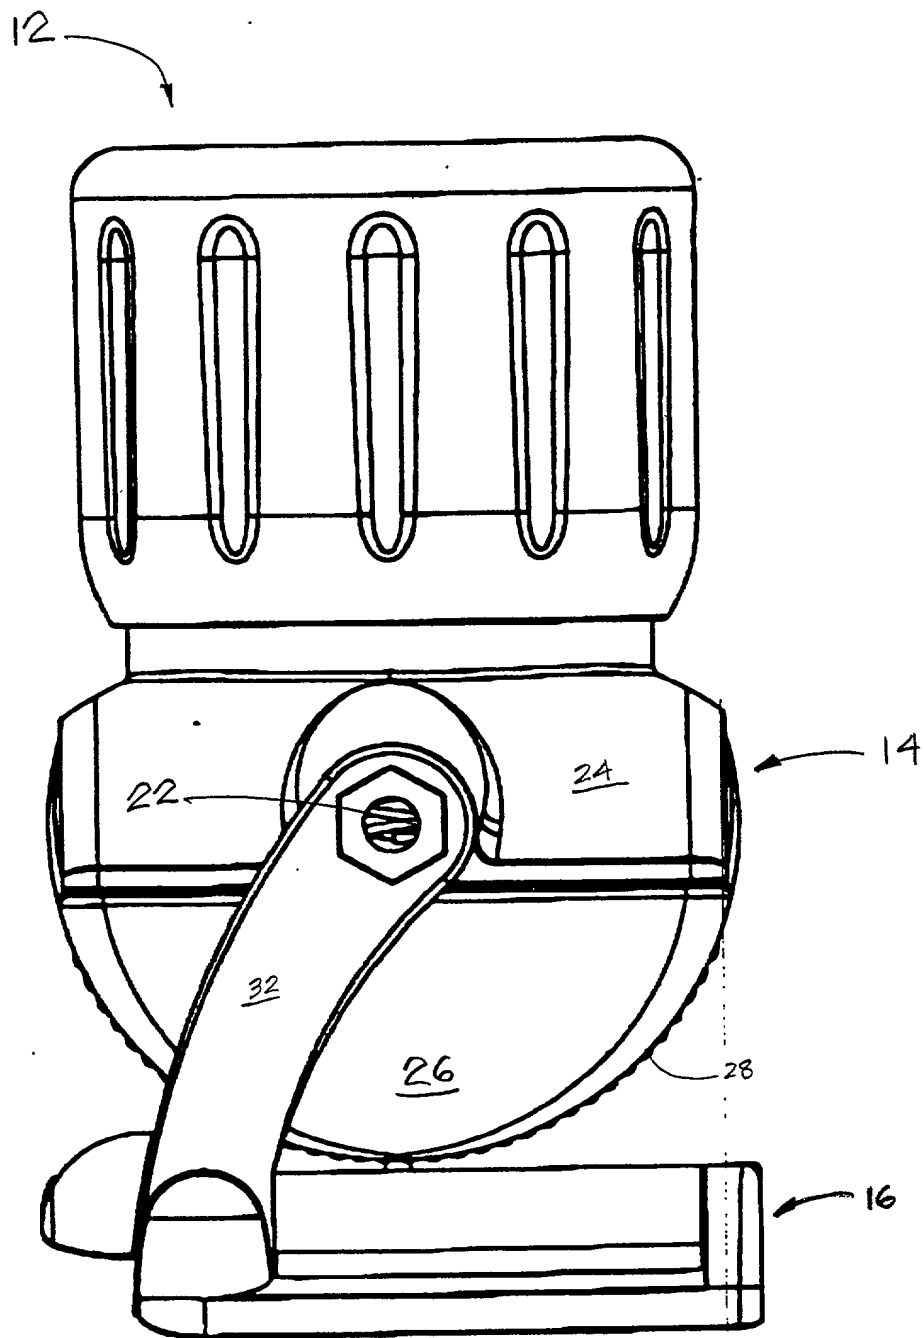


Fig. 5

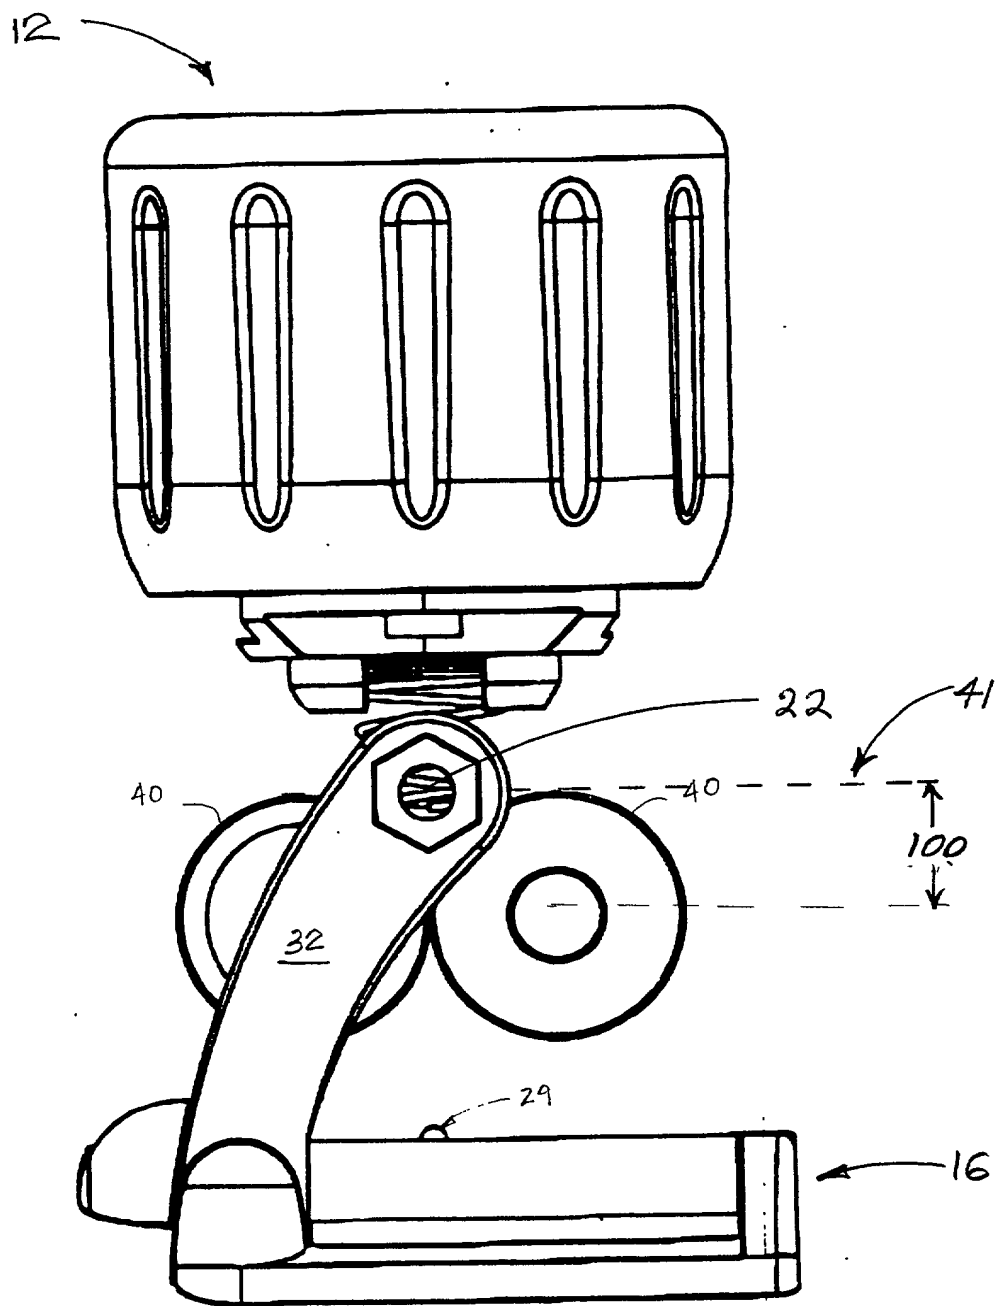


Fig. 6

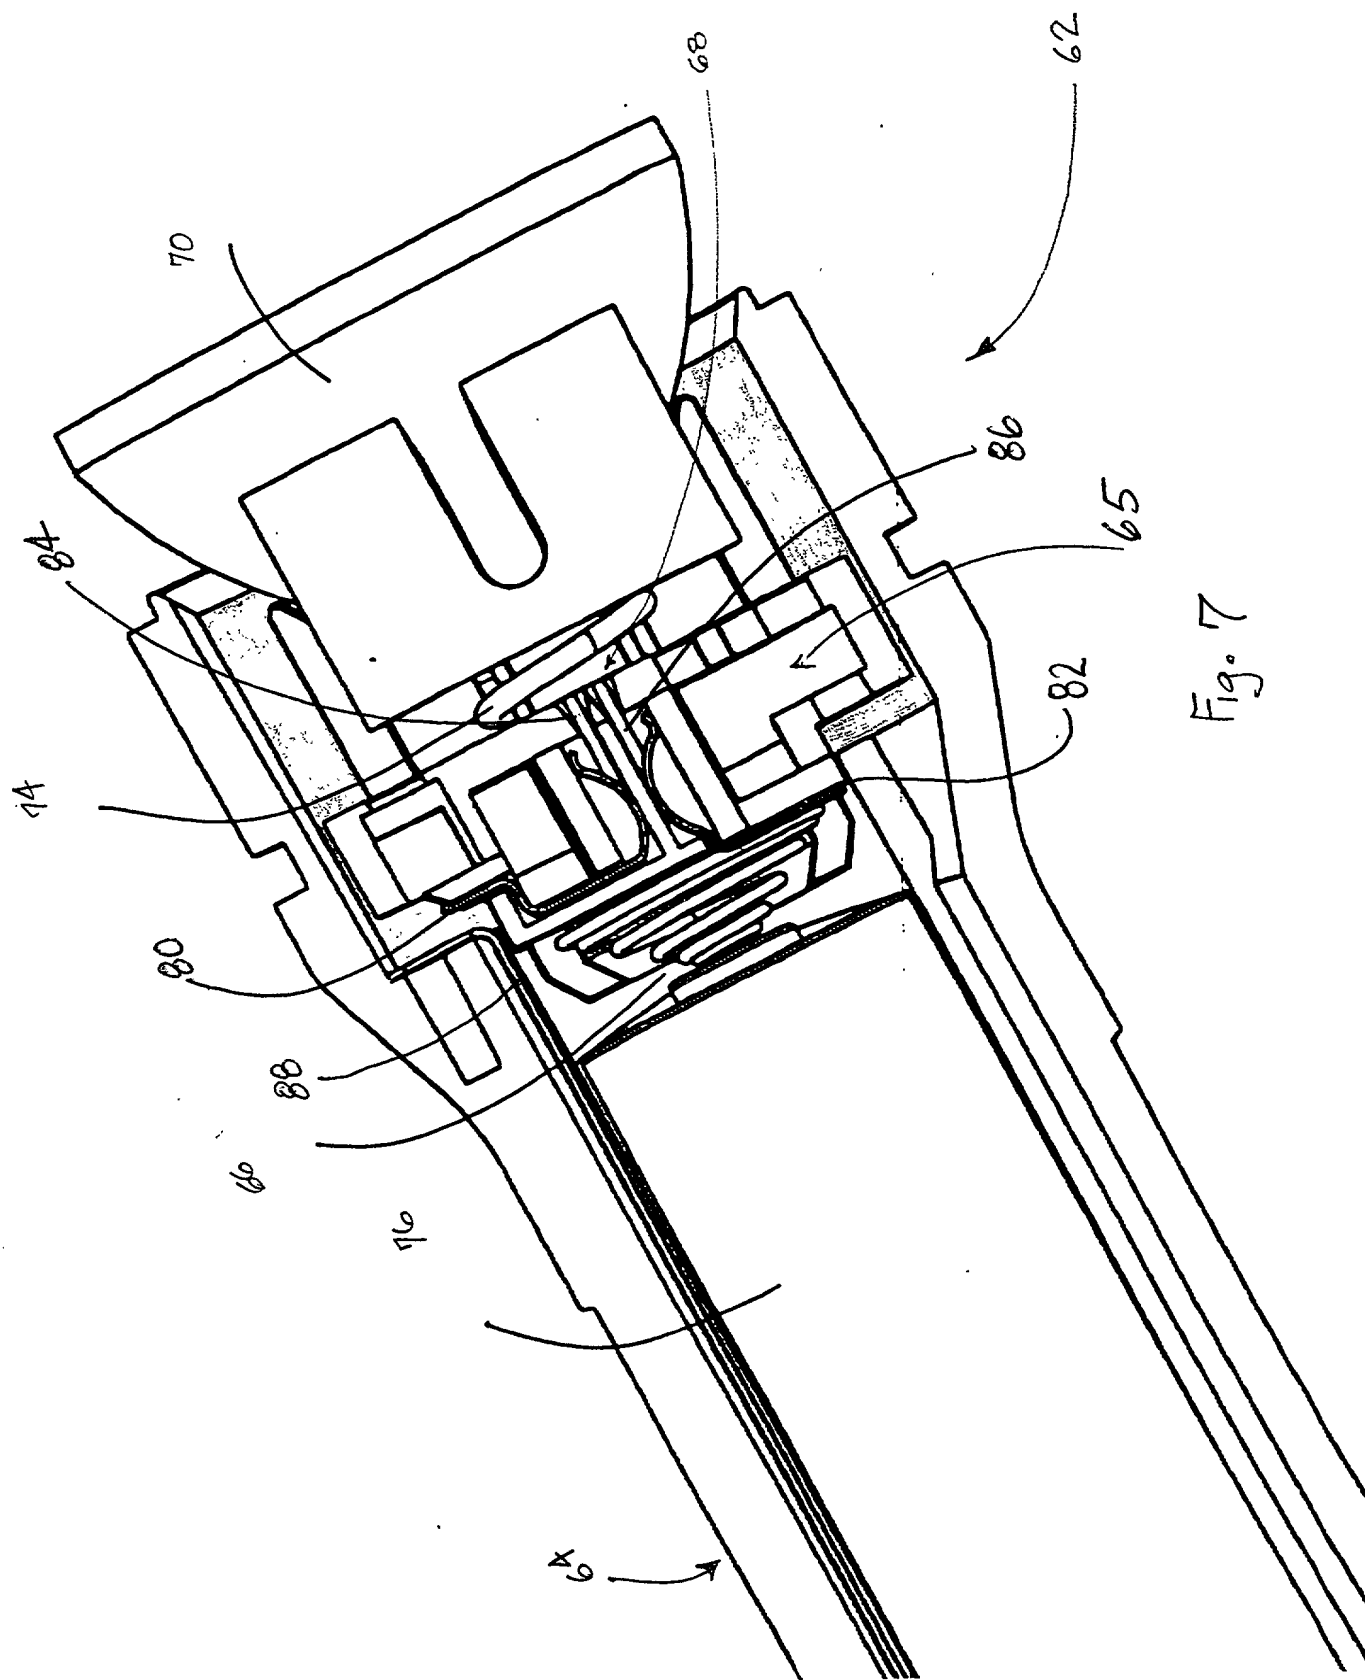


Fig. 7

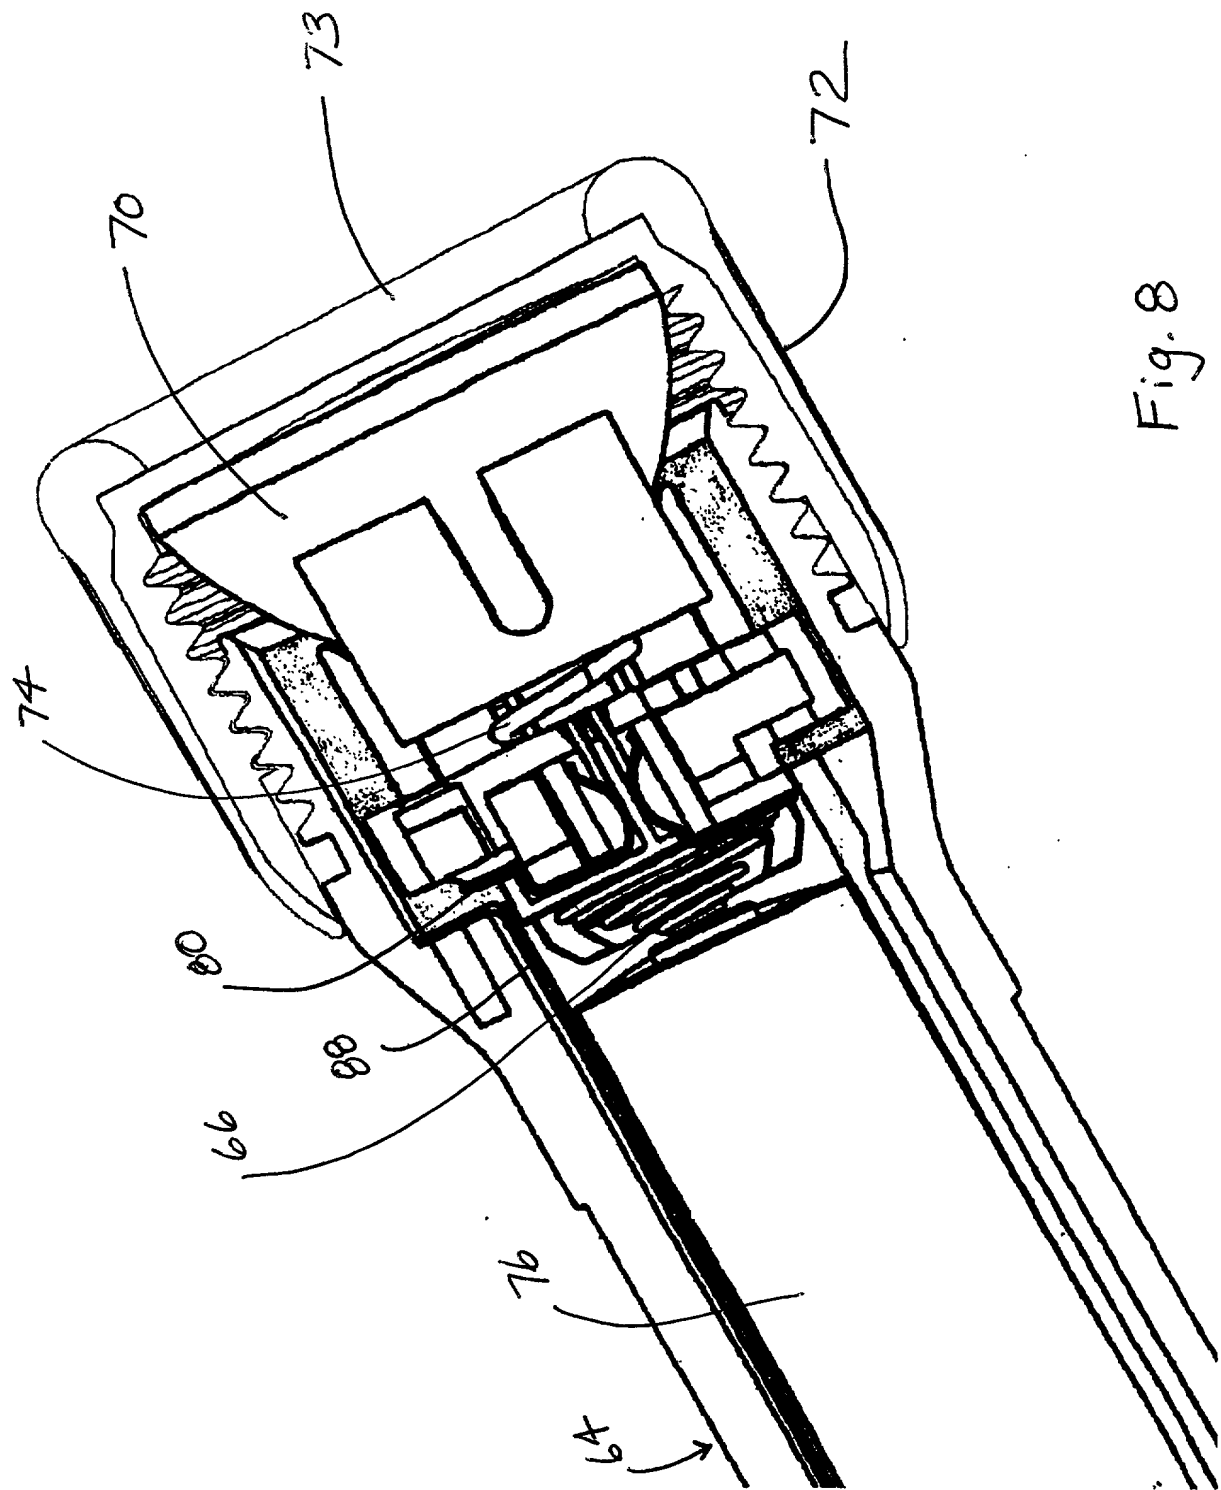


Fig. 8



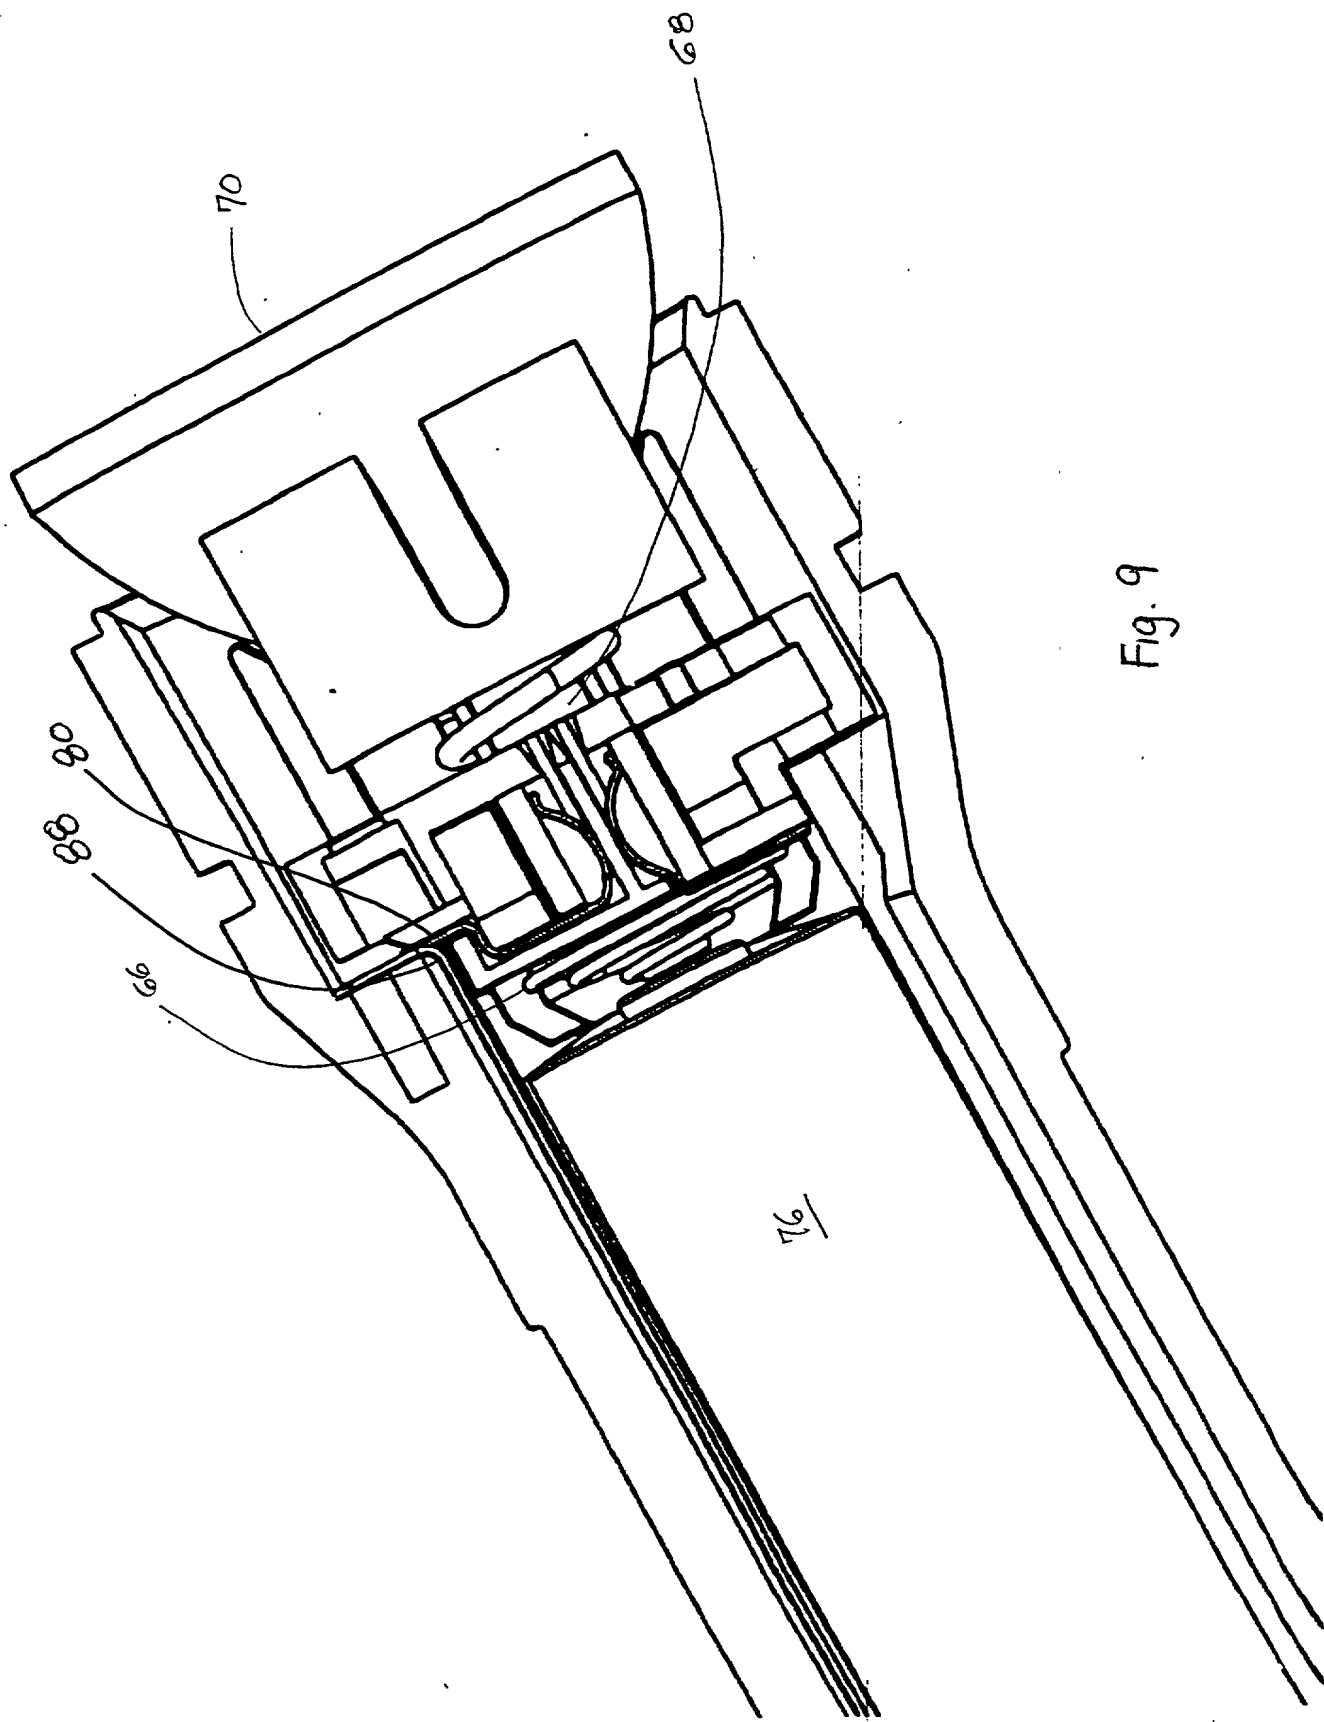


Fig. 9

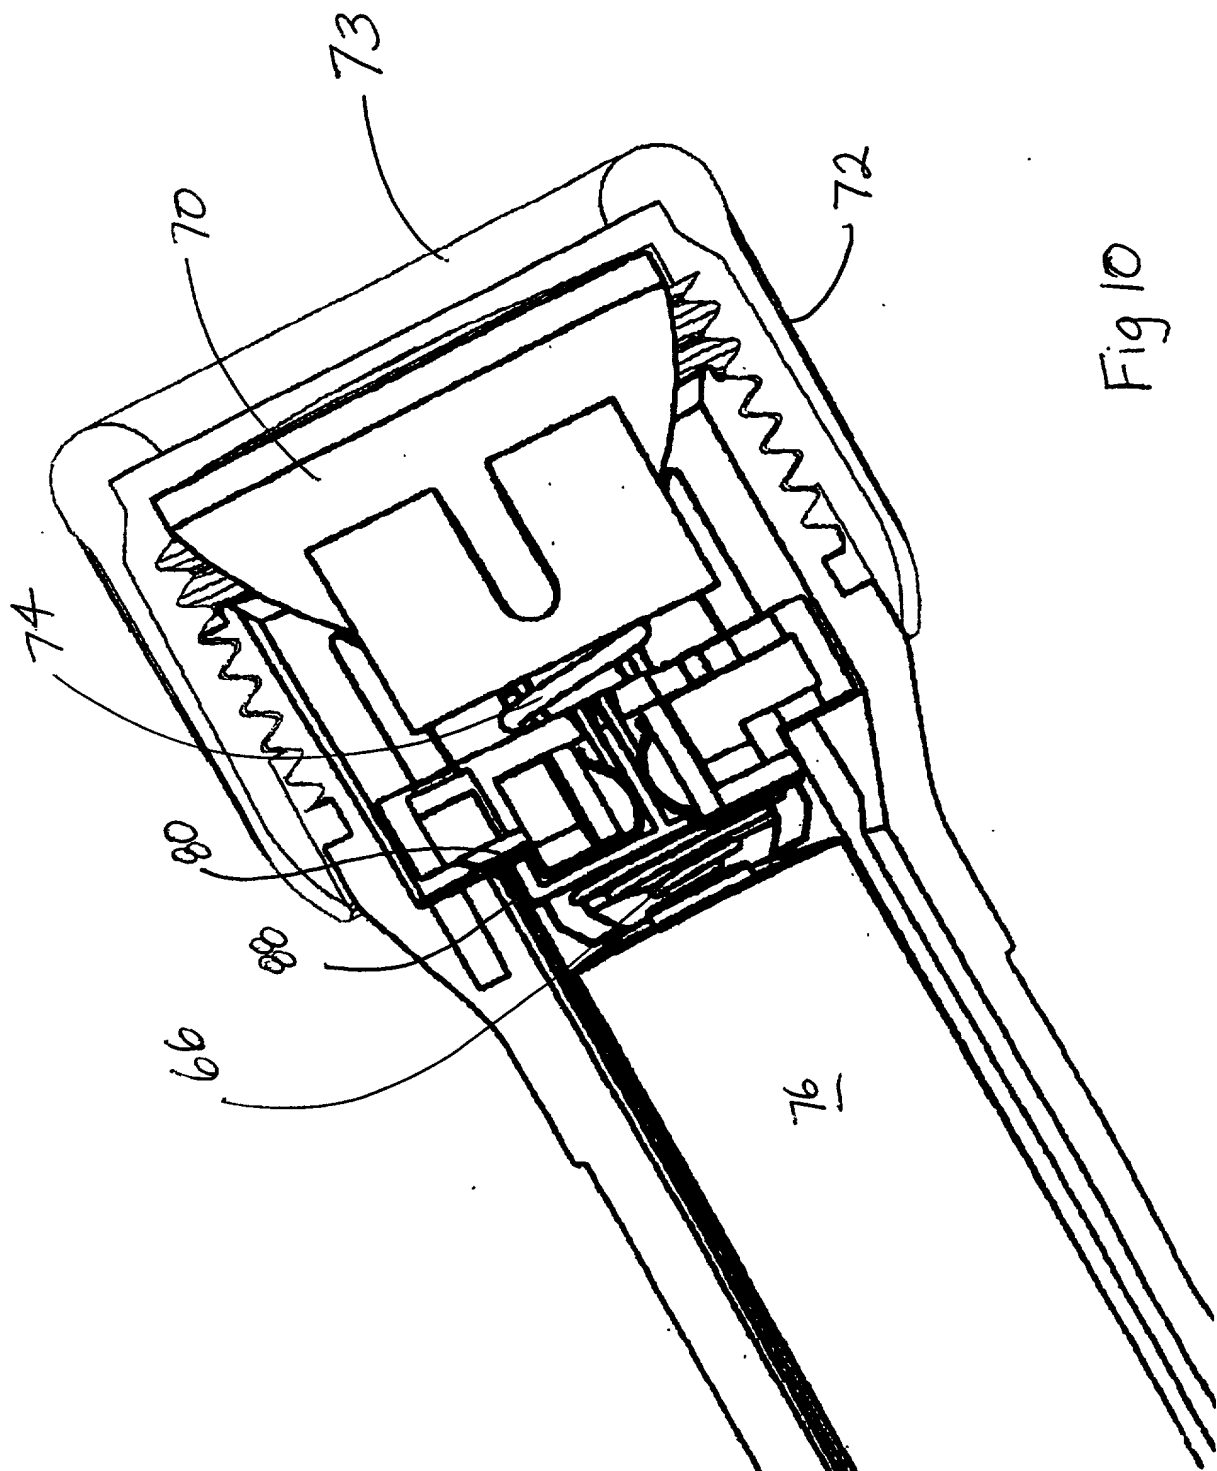


Fig 10

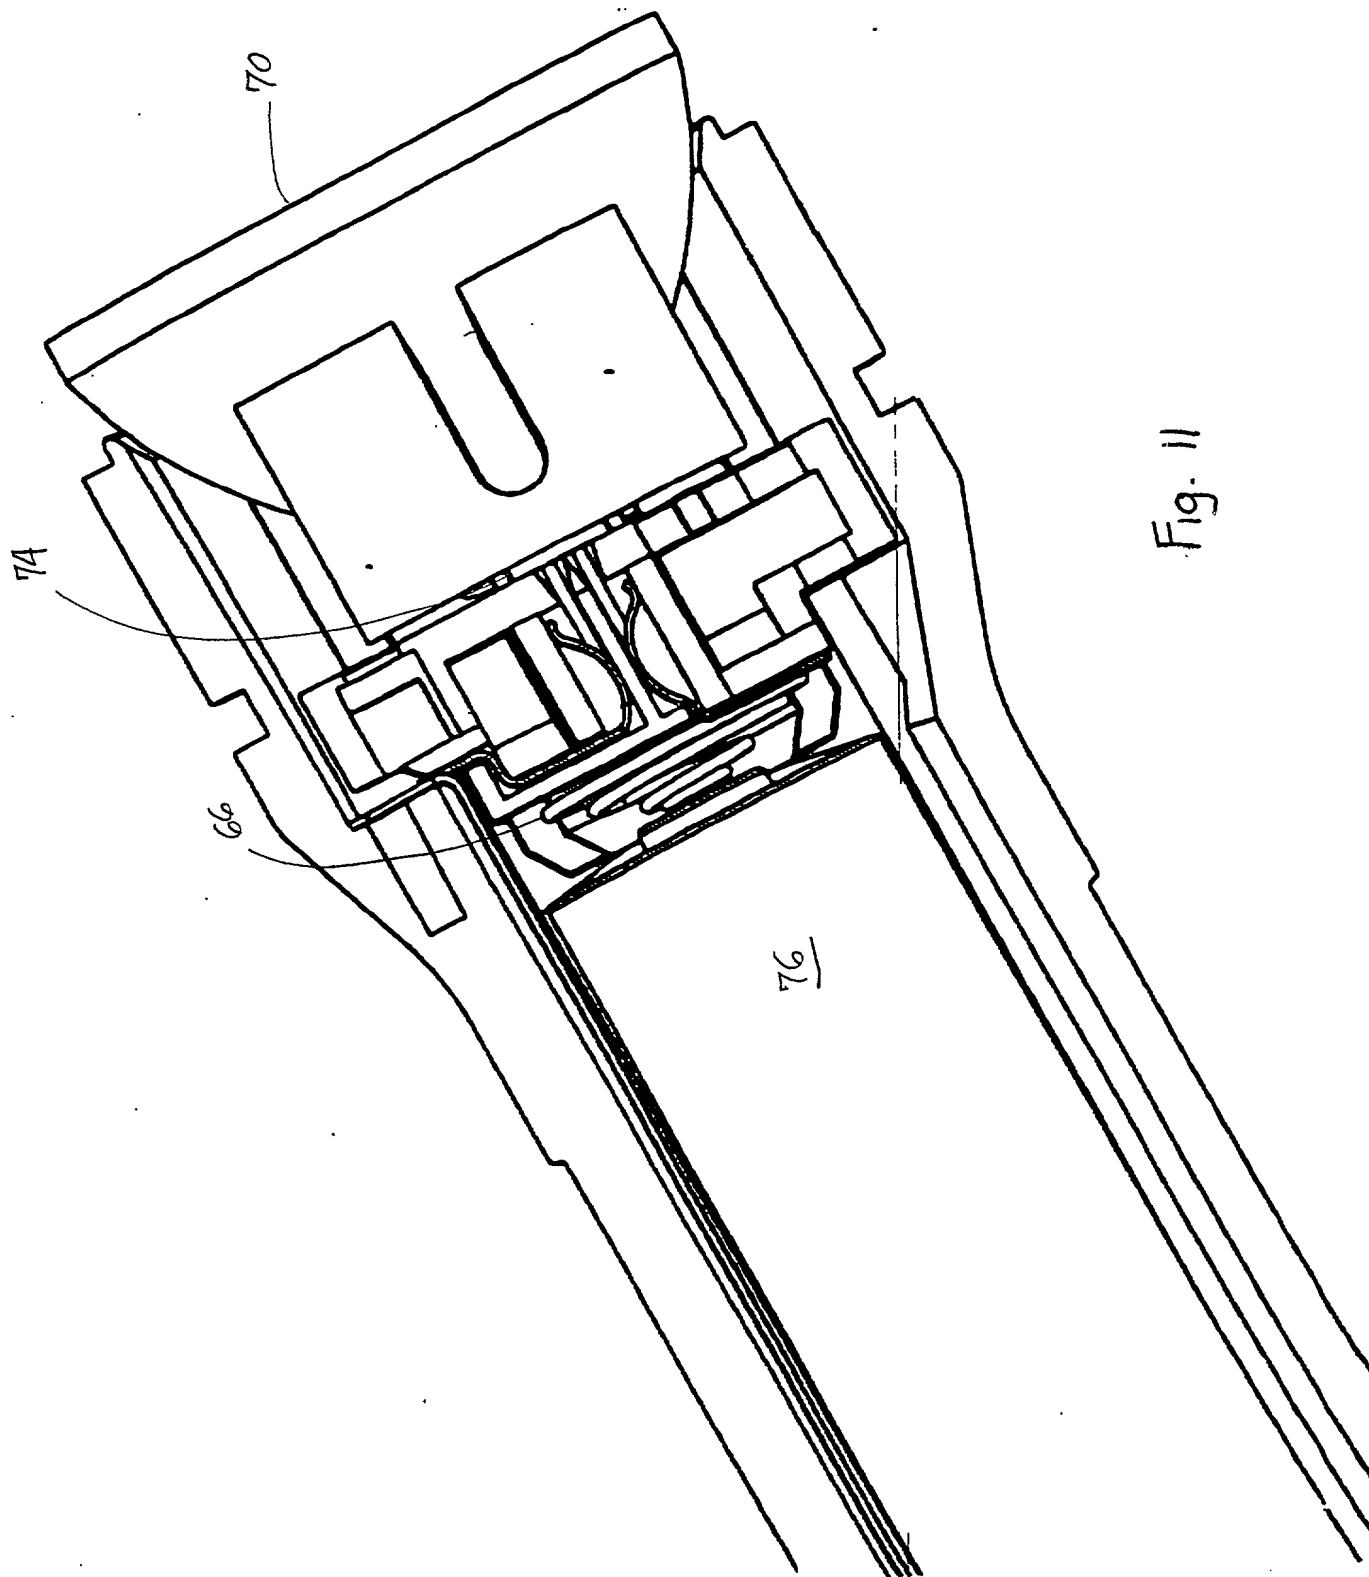


Fig. 11

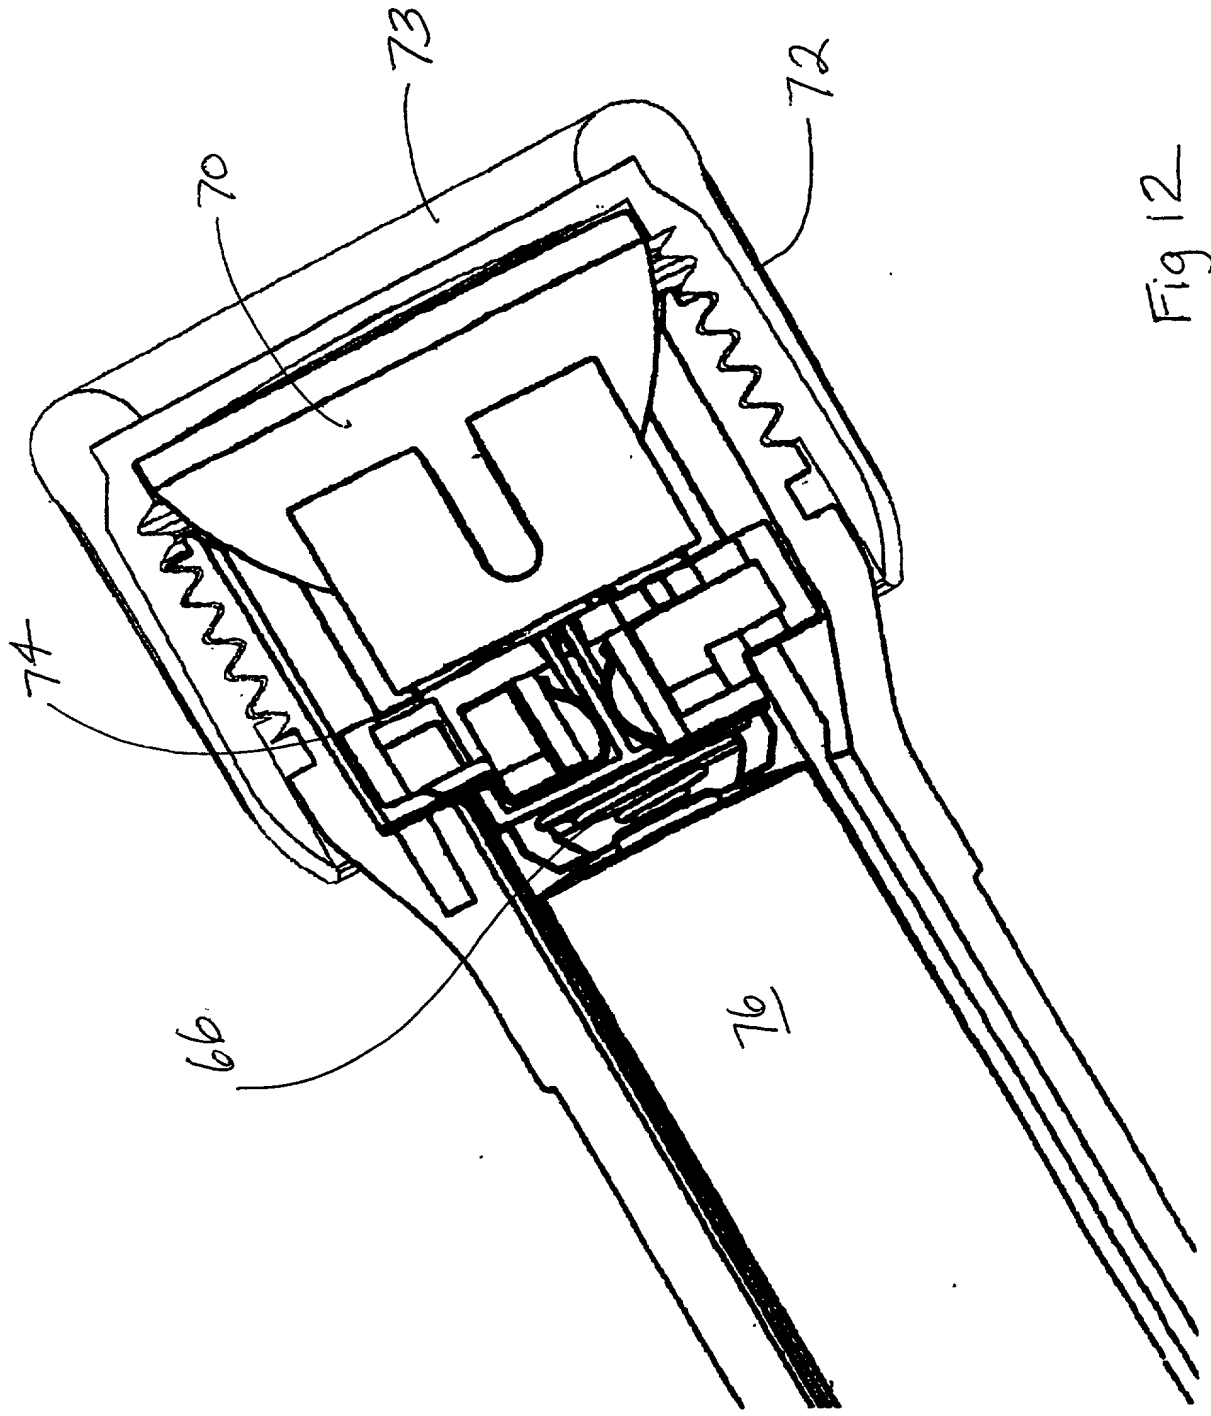


Fig 12